Ordering
Information

External Hex

Dental Implant System

ZimVie

T3® External Hex Implants

D = Diameter • P = Restorative Platform

T3 External Hex Implants

Contemporary Hybrid Surface

T3 Implants: Have a contemporary hybrid design with a T3 surface (blasted and acid-etched with an average surface roughness value of 1.4 µm) along the threaded portion of the implant, and Osseotite® surface (acid-etched) on the collar part of the implant.

T3 Short Implants: Have a full T3 surface.

DCD® Surface: Discrete Crystalline Deposition of nanometer sized calcium phosphate crystals on the dental implant surface.

Material: Commercially pure titanium Grade 4.

T3 External Hex Tapered Implants

Length	3.25 mmD x 3.4 mmP		4.0 mmD x 4.1 mmP		5.0 mmD x 5.0 mmP		6.0 mmD x 6.0 mmP	
	Without DCD	With DCD	Without DCD	With DCD	Without DCD	With DCD	Without DCD	With DCD
8.5 mm	BOET3285	BNET3285	BOET485	BNET485	BOET585	BNET585	BOET685	BNET685
10 mm	BOET3210	BNET3210	BOET410	BNET410	BOET510	BNET510	BOET610	BNET610
11.5 mm	BOET3211	BNET3211	BOET411	BNET411	BOET511	BNET511	BOET611	BNET611
13 mm	BOET3213	BNET3213	BOET413	BNET413	BOET513	BNET513	BOET613	BNET613
15 mm	BOET3215	BNET3215	BOET415	BNET415	BOET515	BNET515	BOET615	BNET615

T3 External Hex Parallel Walled Implants

Length	3.25 mmD x 3.4 mmP		4.0 mmD x 4.1 mmP		5.0 mmD x 5.0 mmP		6.0 mmD x 6.0 mmP	
	Without DCD	With DCD	Without DCD	With DCD	Without DCD	With DCD	Without DCD	With DCD
6.5 mm	BOES365	BNES365	BOES465	BNES465	BOES565	BNES565	BOES665	BNES665
8.5 mm	BOES385	BNES385	BOES485	BNES485	BOES585	BNES585	BOES685	BNES685
10 mm	BOES310	BNES310	BOES410	BNES410	BOES510	BNES510	BOES610	BNES610
11.5 mm	BOES311	BNES311	BOES411	BNES411	BOES511	BNES511	BOES611	BNES611
13 mm	BOES313	BNES313	BOES413	BNES413	BOES513	BNES513	BOES613	BNES613
15 mm	BOES315	BNES315	BOES415	BNES415	BOES515	BNES515	BOES615	BNES615
18 mm	BOES318	BNES318	BOES418	BNES418	N/A	N/A	N/A	N/A

T3 Short Implants

Length	5.0 mmD x 5.0 mmP		6.0 mmD x 6.0 mmP	
	Without DCD	With DCD	Without DCD	With DCD
5 mm	BOES505	BNES505	BOES605	BNES605
6 mm	BOES506	BNES506	BOES606	BNES606

All Implants include the corresponding 1.0 mm height Cover Screw.

Osseotite® External Hex Implants

D = Diameter • P = Restorative Platform

Osseotite External Hex Tapered Implants

Hybrid Osseotite Surface

Full Osseotite Surface

Osseotite Hybrid Dental Implants: Have a hybrid design with a machined collar of 1.25 mm and the Osseotite surface in threaded portion.

Full Osseotite Implants: Have full Osseotite surface in the collar and the threaded portion.

Material: Commercially pure titanium Grade 4.

Osseotite External Hex Tapered Implants

Length	3.25 mmD x 3.4 mmP		4.0 mmD x 4.1 mmP		5.0 mmD x 5.0 mmP		6.0 mmD x 6.0 mmP	
	Hybrid	FOSS	Hybrid	FOSS	Hybrid	FOSS	Hybrid	FOSS
8.5 mm	NT3285	FNT3285	NT485	FNT485	NT585	FNT585	NT685	FNT685
10 mm	NT3210	FNT3210	NT410	FNT410	NT510	FNT510	NT610	FNT610
11.5 mm	NT3211	FNT3211	NT411	FNT411	NT511	FNT511	NT611	FNT611
13 mm	NT3213	FNT3213	NT413	FNT413	NT513	FNT513	NT613	FNT613
15 mm	NT3215	FNT3215	NT415	FNT415	NT515	FNT515	NT615	FNT615

Osseotite External Hex Parallel Walled Implants



Hybrid Osseotite Surface

Full Osseotite Surface

Osseotite Hybrid Implants: Have a hybrid design with a machined collar of 2–3 mm and the Osseotite surface in threaded portion.

Material: Commercially pure titanium Grade 3, except for the 3.25 mmD, which are commercially pure titanium Grade 4.

Full Osseotite Implants: Have full Osseotite surface in the collar and the threaded portion.

Material: Commercially pure titanium Grade 4.

Osseotite External Hex Parallel Walled Implants

Length	3.25 mmD x 3.4 mmP		3.75 mmD x 4.1 mmP		4.0 mmD x 4.1 mmP		5.0 mmD x 5.0 mmP		6.0 mmD x 6.0 mmP	
	Hybrid	FOSS	Hybrid	FOSS	Hybrid	FOSS	Hybrid	FOSS	Hybrid	FOSS
7.0 mm	N/A	XFOSM365	N/A	XFOS365	N/A	XFOS465	OSS507	XFOS565	OSS607	XFOS665
8.5 mm	OSM385	XFOSM385	OSS385	XFOS385	OSS485	XFOS485	OSS585	XFOS585	OSS685	XFOS685
10 mm	OSM310	XFOSM310	OSS310	XFOS310	OSS410	XFOS410	OSS510	XFOS510	OSS610	XFOS610
11.5 mm	OSM311	XFOSM311	OSS311	XFOS311	OSS411	XFOS411	OSS511	XFOS511	OSS611	XFOS611
13 mm	OSM313	XFOSM313	OSS313	XFOS313	OSS413	XFOS413	OSS513	XFOS513	OSS613	XFOS613
15 mm	OSM315	XFOSM315	OSS315	XFOS315	OSS415	XFOS415	OSS515	XFOS515	OSS615	XFOS615
18 mm	OSM318	N/A	OSS318	N/A	OSS418	N/A	OSS518	N/A	OSS618	N/A
20 mm	N/A	N/A	OSS320	N/A	OSS420	N/A	N/A	N/A	N/A	N/A

Full Osseotite Parallel Walled Implants

Length	3.25 mmD x 3.4 mmP	3.75 mmD x 4.1 mmP	4.0 mmD x 4.1 mmP	5.0 mmD x 5.0 mmP	6.0 mmD x 6.0 mmP
7.0 mm	FOSM307	FOS307	FOS407	FOS507	FOS607
8.5 mm	FOSM385	FOS385	FOS485	FOS585	FOS685
10 mm	FOSM310	FOS310	FOS410	FOS510	FOS610
11.5 mm	FOSM311	FOS311	FOS411	FOS511	FOS611
13 mm	FOSM313	FOS313	FOS413	FOS513	FOS613
15 mm	FOSM315	FOS313	FOS415	FOS515	FOS615

All implants include the corresponding 1.0 mm height Cover Screw.

Healing Abutments

P = Restorative Platform • EP = Emergence Profile • H = Collar Height
PS = Platform Switched • NPS = Non-Platform Switched

Color Coding

External Hex Implants have a color-coded restorative platform with four different seating surfaces: 3.4 mm, 4.1 mm, 5.0 mm, and 6.0 mm. The hex size of the 4.1 mm, 5.0 mm, and 6.0 mm is the same.

3.4 mm Restorative Platform | 4.1 mm Restorative Platform | 5.0 mm Restorative Platform | 6.0 mm Restorative Platform

Three different Emergence Profiles for the same Restorative Platform

Material: Titanium Alloy

Encode® Healing Abutments

3.4 mmP Restorative Platform

Description	Item #
3.8 mmEP x 3.0 mmH	EHA343
3.8 mmEP x 4.0 mmH	EHA344
3.8 mmEP x 6.0 mmH	EHA346
3.8 mmEP x 8.0 mmH	EHA348
5.0 mmEP x 3.0 mmH	EHA353
5.0 mmEP x 4.0 mmH	EHA354
5.0 mmEP x 6.0 mmH	EHA356
5.0 mmEP x 8.0 mmH	EHA358



4.1 mmP Restorative Platform

Description	Item #
4.1 mmEP x 3.0 mmH	EHA443
4.1 mmEP x 4.0 mmH	EHA444
4.1 mmEP x 6.0 mmH	EHA446
4.1 mmEP x 8.0 mmH	EHA448
5.0 mmEP x 3.0 mmH	EHA453
5.0 mmEP x 4.0 mmH	EHA454
5.0 mmEP x 6.0 mmH	EHA456
5.0 mmEP x 8.0 mmH	EHA458
6.0 mmEP x 3.0 mmH	EHA463
6.0 mmEP x 4.0 mmH	EHA464
6.0 mmEP x 6.0 mmH	EHA466
6.0 mmEP x 8.0 mmH	EHA468

Encode Healing Abutments are two pieces.

5.0 mmP Restorative Platform

Description	Item #
5.6 mmEP x 3.0 mmH	EHA553
5.6 mmEP x 4.0 mmH	EHA554
5.6 mmEP x 6.0 mmH	EHA556
5.6 mmEP x 8.0 mmH	EHA558
6.0 mmEP x 3.0 mmH	EHA563
6.0 mmEP x 4.0 mmH	EHA564
6.0 mmEP x 6.0 mmH	EHA566
6.0 mmEP x 8.0 mmH	EHA568

6.0 mmP Restorative Platform

Description	Item #
6.8 mmEP x 3.0 mmH	EHA663
6.8 mmEP x 4.0 mmH	EHA664
6.8 mmEP x 6.0 mmH	EHA666
6.8 mmEP x 8.0 mmH	EHA668

Occlusal markings provide information designed to aid in the design of patient specific abutments.

Standard EP® Healing Abutments

3.4 mmP Restorative Platform

Description	Item #
3.8 mmEP x 2.0 mmH	MHA32
3.8 mmEP x 3.0 mmH	MHA33
3.8 mmEP x 4.0 mmH	MHA34
3.8 mmEP x 6.0 mmH	MHA36

4.1 mmP Restorative Platform

Description	Item #
4.1 mmEP x 2.0 mmH	THA42
4.1 mmEP x 3.0 mmH	THA43
4.1 mmEP x 4.0 mmH	THA44
4.1 mmEP x 6.0 mmH	THA46
4.1 mmEP x 8.0 mmH	THA48
5.0 mmEP x 2.0 mmH	THA52
5.0 mmEP x 3.0 mmH	THA53
5.0 mmEP x 4.0 mmH	THA54
5.0 mmEP x 6.0 mmH	THA56
5.0 mmEP x 8.0 mmH	THA58
6.0 mmEP x 3.0 mmH	THA63
6.0 mmEP x 4.0 mmH	THA64
6.0 mmEP x 6.0 mmH	THA66
6.0 mmEP x 8.0 mmH	THA68

Standard Healing Abutments are one piece.

5.0 mmP Restorative Platform

Description	Item #
5.6 mmEP x 2.0 mmH	WTH52
5.6 mmEP x 3.0 mmH	WTH53
5.6 mmEP x 4.0 mmH	WTH54
5.6 mmEP x 6.0 mmH	WTH56
5.6 mmEP x 8.0 mmH	WTH58
6.0 mmEP x 2.0 mmH	WTH562
6.0 mmEP x 3.0 mmH	WTH563
6.0 mmEP x 4.0 mmH	WTH564
6.0 mmEP x 6.0 mmH	WTH566
6.0 mmEP x 8.0 mmH	WTH568

6.0 mmP Restorative Platform

Description	Item #
6.8 mmEP x 2.0 mmH	WTH62
6.8 mmEP x 3.0 mmH	WTH63
6.8 mmEP x 4.0 mmH	WTH64
6.8 mmEP x 6.0 mmH	WTH66
6.8 mmEP x 8.0 mmH	WTH68

Provisional Restorations

P = Restorative Platform
EP = Emergence Profile • H = Collar Height

Temporary Cylinders

Material: PEEK Plastic or titanium alloy

Indications:

- Single- and multiple-unit provisional screw-retained restorations
- Minimum interarch space of 6 mm for PreFormance and 7 mm for Titanium Cylinders
- Maximum angulation of 15°
- Intraoral use limited to 180 days for the PreFormance Temporary Cylinders
- Immediate non-occlusal loading of single-unit provisional restorations
- Multiple-unit restorations will require an evaluation of occlusal forces in lateral and protrusive excursions and masticatory forces to minimize the load on the provisional restorations

PreFormance Temporary Cylinders

Restorative Platform	Item # (Hexed)	Item # (Non-Hexed)
3.4 mmP	MPFTC34	MPFTC32
4.1 mmP	PFTC41	PFTC42
5.0 mmP	WPFTC51	WPFTC52
6.0 mmP	WPFTC61	WPFTC62

Titanium Temporary Cylinders

Restorative Platform	Item # (Hexed)	Item # (Non-Hexed)
3.4 mmP	MMTCS1	MMTCS2*
4.1 mmP	ITCS41	ITCS42
5.0 mmP	WTCS51	WTCS52
6.0 mmP	WTCS61	WTCS62

All Temporary Cylinders include the corresponding Titanium Hexed Screw.
* Screw not included. MMTCS2 is not available in all markets. Please contact your local sales representative.

Definitive Restorations

P = Restorative Platform • EP = Emergence Profile • H = Collar Height

GingiHue® Posts

Material: Titanium alloy with titanium nitride coating

Indications:

- Single- and multi-unit cement-retained restorations
- Areas of thin tissue where gingival discoloration is possible
- Preparable to follow gingival contours
- Conventional crown and bridge procedures
- Maximum angulation correction of 15°
- Minimum interarch space of 6.0 mm

The 12-point double hex, which is machined in the 15° Pre-Angled GingiHue Abutment, provides rotational positioning in 30° increments on the implant hex.

GingiHue Posts

3.4 mmP Restorative Platform

Description	Item # (Straight)	Item # (15° Pre-Angled)
3.8 mmEP x 2.0 mmH	MAP32G	MPAP32G
3.8 mmEP x 4.0 mmH	MAP34G	MPAP34G

4.1 mmP Restorative Platform

Description	Item # (Straight)	Item # (15° Pre-Angled)
5.0 mmEP x 2.0 mmH	APP452G	PAP452G
5.0 mmEP x 4.0 mmH	APP454G	PAP454G
6.0 mmEP x 2.0 mmH	APP462G	PAP462G
6.0 mmEP x 4.0 mmH	APP464G	PAP464G

5.0 mmP Restorative Platform

Description	Item # (Straight)	Item # (15° Pre-Angled)
5.0 mmEP x 2.0 mmH	WPP552G	PAP552G
5.0 mmEP x 4.0 mmH	WPP554G	PAP554G
6.0 mmEP x 2.0 mmH	WPP562G	PAP562G
6.0 mmEP x 4.0 mmH	WPP564G	PAP564G

6.0 mmP Restorative Platform

Description	Item # (Straight)	Item # (15° Pre-Angled)
6.0 mmEP x 2.0 mmH	WPP662G	PAP662G
6.0 mmEP x 4.0 mmH	WPP664G	PAP664G

GingiHue Posts do not include the screw. The final Gold-Tite® Screw (UNISG) must be ordered separately.

GenTek® Ti-Bases® with Standard PO, Sirona inCoris Meso Block/ Cerec Compaitble

- Cement- and screw-retained restorations
- Single- and multi-unit restorations
- Traditional workflow or CAD/CAM digital workflow with scan posts

GenTek Ti-Bases

Height 4.7 mmP

Description	Item # (Engaging)	Item # (Non-Engaging)
3.4 mm	ZFX11-ZB-EX-3447-EL	ZFX11-ZB-EX-3447-NEL
4.1 mm	ZFX11-ZB-EX-4147-EL	ZFX11-ZB-EX-4147-NEL
5.0 mm	ZFX11-ZB-EX-5047-EL	ZFX11-ZB-EX-5047-NEL

GenTek Scan Bodies

Description	Item # (Engaging)	Item # (Non-Engaging)
3.4 mm	IOS Scan Body	ZFX-05Z-ZB-EX-31
4.1 mm	IOS Scan Body	ZFX-05Z-ZB-EX-41
5.0 mm	IOS Scan Body	ZFX-05Z-ZB-EX-50
6.0 mm	IOS Scan Body	ZFX-05Z-ZB-EX-60



All GenTek Ti-Bases include the incl. Gold-Tite and Gluing Screws

* Not available in all markets. Please contact your local sales representative.

GemLock Screwdriver

Description	Item #
Hex Driver, Long, with GemLock Retention 1.25 mmD, 30 mmL	HXLGR1.25

GenTek Ti-Bases - Screws

Description	Item #
Gold-Tite Screw / 32Ncm	ZFX09-ZB-EX-GTS
Titanium Try-In Screw / Handtighten	ZFX09-ZB-EX-TIS

Square Driver, Driver Tip
for Gold-Tite Screw

Description	Item #
Narrow Posterior Square Driver, 17 mmL	PSQD0N
Narrow Standard Slotted Square Driver, 24 mmL	PSQD1N
Narrow Right Angle Square Driver Tip, 24 mmL	RASQ3N

Hex Driver, Driver Tip
for Try-In Screw

Description	Item #
Narrow Posterior Hex Driver, 17 mmL	PHD02N
Narrow Standard Hex Driver, 24 mmL	PHD03N
Latch-Lock Hex Driver Tip With GemLock Retention 1.2 mm(D) 24 mm(L)	IHX1.2D
Latch-Lock Hex Driver Tip With GemLock Retention 1.2 mm(D) 30 mm(L)	IXL1.2D

P = Restorative Platform

UCLA Abutments

Material:
- Gold: Machined gold allow cylinder with plastic unitube
- Castable: Delrin plastic
- Titanium: Titanium alloy

Indications:
- Cement- and screw-retained restorations
- Single- and multi-unit restorations
- Laboratory fabricated custom abutments and bridges
- For aesthetic restorations when tissue is limited
- Maximum angulation correction of 30°
- Minimum interarch space of 6.0 mm

Gold Standard ZR (Zero Rotation) is a proprietary design incorporating machined microstops within the corners of the hex in the abutment. The design reduces horizontal rotation between the implant and abutment. Gold Standard ZR is available on UCLA and GingiHue Hexed Abutments.

UCLA Abutment*

3.4 mmP Restorative Platform

Material	Hexed	Non-Hexed
Gold	MUCG1C	MUCG2C
Castable - Plastic	MUCC1C	MUCC2C

4.1 mmP Restorative Platform

Material	Hexed	Non-Hexed
Gold	SGUCA1C	GUCA2C
Castable - Plastic	UNAB1C	UNAB2C
Titanium Laser Welding	TUCA1C	TUCA2C

5.0 mmP Restorative Platform

Material	Hexed	Non-Hexed
Gold	SWGA51C	WGA52C
Castable - Plastic	WPC51C	WPC52C

6.0 mmP Restorative Platform

Material	Hexed	Non-Hexed
Gold	SWGA61C	WGA62C
Castable - Plastic	WPC61C	WPC62C

*Non-Hexed UCLA Abutments are used for multiple-unit screw-retained restorations. The UCLA Abutment does not include the screw. The final Gold-Tite Screw (UNIHG/UNISG) or the Titanium Screw (UNIHT) must be ordered separately.

Gold Alloy Cylinder Formulation	
Melting Range	1400–1490°C (2550–2710°F)
Solidus	1400°C
Liquidus	1490°C
An alloy with a CTE of 10·°K at 500°C is recommended for casting.	

Definitive Restorations

P = Restorative Platform • H = Collar Height • L = Length

Low Profile Abutments

Material: Titanium alloy

Indications:

- Two-piece abutments for single-unit screw-retained restorations
- One-piece abutments for multi-unit screw-retained restorations
- Minimum interarch space of 7.5 mm
- Minimum tissue height of 1.0 mm
- Maximum angulation correction of 30°

The Low Profile Abutments are conveniently packaged with the ASYST Abutment Placement Tool. Temporary cylinders do not include screw (require LPCGSH or LPCTSH)

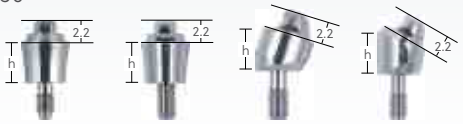

Low Profile Abutments

3.4 mmP Restorative Platform

Description	One Piece	Two Piece	17°	30°
1.0 mmH	LPC341U	LPC341	–	–
2.0 mmH	LPC342U	LPC342	LPAC3217	–
3.0 mmH	LPC343U	LPC343	–	LPAC3330
4.0 mmH	LPC344U	LPC344	LPAC3417	–
5.0 mmH	–	–	–	LPAC3530

4.1 mmP Restorative Platform

Description	One Piece	Two Piece	17°	30°
1.0 mmH	LPC441U	LPC441	–	–
2.0 mmH	LPC442U	LPC442	LPAC4217	–
3.0 mmH	LPC443U	LPC443	–	LPAC4330
4.0 mmH	LPC444U	LPC444	LPAC4417	–
5.0 mmH	–	–	–	LPAC4530

5.0 mmP Restorative Platform

Description	One Piece	Two Piece	17°	30°
1.0 mmH	LPC541U	LPC541	–	–
2.0 mmH	LPC542U	LPC542	LPAC5217	–
3.0 mmH	LPC543U	LPC543	–	LPAC5330
4.0 mmH	LPC544U	LPC544	LPAC5417	–
5.0 mmH	–	–	–	LPAC5530

Component/Abutment Compatibility

Component	Hexed Abutment	Non-Hexed Abutment
Hexed	Yes	No
Non-Hexed	Yes	Yes

Low Profile Retaining Screws

Description	Item #
Gold-Tite Low Profile Retaining Screw	LPCGSH
Titanium Low Profile Retaining Screw	LPCTSH
Waxing Low Profile Screw	LPCWS

Low Profile Impression Copings and Analog

Description	Item #
Pick Up Impression Coping (Hexed)	LPCPIC1
Pick Up Impression Coping (Non-Hexed)	LPCPIC2
Twist Lock™ Impression Coping (Hexed)	LPCTIC1
Twist Lock Impression Coping (Non-Hexed)	LPCTIC2
QuickBridge® Impression Coping	LPCRIC
Laboratory Analog	LPCLA

Low Profile Final Restoration Components

Description	Item #
Gold Cylinder (Hexed)	LPCGC1
Gold Cylinder (Non-Hexed)	LPCGC2
Castable Cylinder (Hexed)	LPCCC1
Castable Cylinder (Non-Hexed)	LPCCC2
Titanium Laser Welded Cylinder	LPCTUCA

Low Profile Laboratory Tools

Description	Item #
Low Profile Lapping Tool	LPCAMI
Low Profile Polishing Protector	LPCPP

Low Profile Provisional Restoration Components

Description	Item #
Titanium Temporary Cylinder (Hexed)	LPCTC1
Titanium Temporary Cylinder (Non-Hexed)	LPCTC2
PreFormance Temporary Cylinder (Hexed)	LPCPTC1
PreFormance Temporary Cylinder (Non-Hexed)	LPCPTC2
Healing Cap	LPCHC
QuickBridge Cylinder	LPCQB
QuickBridge Cap	LPCQBCAP
Distal Extension	LPCDE

Temporary cylinders do not include screw (require LPCGSH or LPCTSH)

Drivers and Tips

Description	Item #
Low Profile Abutment Driver Short (17 mmL) and Long (24 mmL)	PAD00, PAD24
Hexed Driver Short (17 mm) and Long (24 mmL)	PHD02N, PHD03N
Latch-Lock Hex Driver Tip with GemLock Retention 1.2 mm(D): 24 mm(L) and 30 mm(L)	IHX1.2D, IXL1.2D
Low Profile Abutment Driver Tip	RASA3

Overdenture Restorations

P = Restorative Platform • H = Collar Height • L = Length

OverdenSURE® Abutments

Material:
Abutment: Titanium alloy with zirconium nitride coating
Housing: Titanium alloy. Inserts: Nylon

Indications:
- Tissue supported removable overdentures on 2-4 implants
- Partially edentulous overdentures with one or more implants
- Limited interarch distance
- Angle correction up to 40° between divergent implants

All markets outside the U.S.

External Hex Implant System			
Collar Height	Seating Surface		
	3.4 mm	4.1 mm	5.0 mm
1.0 mm	ODS-EXHEX301	ODS-EXHEX401	ODS-EXHEX501
2.0 mm	ODS-EXHEX302	ODS-EXHEX402	ODS-EXHEX502
3.0 mm	ODS-EXHEX303	ODS-EXHEX403	ODS-EXHEX503
4.0 mm	ODS-EXHEX304	ODS-EXHEX404	ODS-EXHEX504
5.0 mm	ODS-EXHEX305	ODS-EXHEX405	ODS-EXHEX505
6.0 mm	ODS-EXHEX306	ODS-EXHEX406	ODS-EXHEX506

OverdenSURE Attachments

All markets outside the U.S.

Description	Item No.
Retention Kit 20° Qty 1 Set	ODS-RIKIT2001
Retention Kit 20° Qty 2 Sets	ODS-RIKIT2002
Retention Kit 40° Qty 1 Set	ODS-RIKIT4001
Retention Kit 40° Qty 2 Sets	ODS-RIKIT4002
Blue Retention Insert 20° Qty 4	ODS-RIB2004
Pink Retention Insert 20° Qty 4	ODS-RIP2004
Clear Retention Insert 20° Qty 4	ODS-RIC2004
Red Retention Insert 40° Qty 4	ODS-RIR4004
Yellow Retention Insert 40° Qty 4	ODS-RIY4004
Green Retention Insert 40° Qty 4	ODS-RIG4004

OverdenSURE Tools and Accessories

Description	Item No.
Retention Housing Cap Qty 1	ODS-RH01
Retention Housing Cap Qty 4	ODS-RH04
Retention Housing Cap Qty 10	ODS-RH010
Blockout Spacer Qty 20	ODS-BS020
Abutment Driver	ODS-DRVR
Removal and Insertion Tool	ODS-IRTOOL
Impression Coping Qty 1	ODS-IC01
Impression Coping Qty 4	ODS-IC04
Impression Coping Qty 10	ODS-IC010
Abutment Bar Attachment Qty 1	ODS-BARATT01**
Abutment Bar Attachment Qty 2	ODS-BARATT02**
Abutment Bar Attachment Qty 4	ODS-BARATT04**
Analog Qty 1	ODS-AA01
Analog Qty 4	ODS-AA04
Analog Qty 10	ODS-AA010

** Retention Kits not included

Impression Copings, Laboratory Analogs, Drivers, and Screws

P = Restorative Platform • EP = Emergence Profile • D = Diameter

Pick-Up Impression Copings

3.4 mmP	Restorative Platform
Emergence Profile	Item #
3.8 mmEP	MIC33

4.1 mmP	Restorative Platform
Emergence Profile	Item #
4.1 mmEP	IIC41
5.0 mmEP	IIC12
6.0 mmEP	IIC60

5.0 mmP	Restorative Platform
Emergence Profile	Item #
5.6 mmEP	WIP55
6.0 mmEP	WIP56

6.0 mmP	Restorative Platform
Emergence Profile	Item #
6.8 mmEP	WIP66

Twist Lock™ Impression Copings

4.1 mmP	Restorative Platform
Emergence Profile	Item #
5.0 mmEP	IIC45
6.0 mmEP	IIC46

5.0 mmP	Restorative Platform
Emergence Profile	Item #
5.0 mmEP	WIT55
6.0 mmEP	WIT56

6.0 mmP	Restorative Platform
Emergence Profile	Item #
6.0 mmEP	WIT66

Implant Laboratory Analogs

3.4 mmP	Restorative Platform
Description	Item #
Lab Analog	MMILA

4.1 mmP	Restorative Platform
Description	Item #
Lab Analog	ILA20

5.0 mmP	Restorative Platform
Description	Item #
Lab Analog	ILAW5

6.0 mmP	Restorative Platform
Description	Item #
Lab Analog	ILAW6

Torque Driver Kits

Description	Item #
Low Torque Indicating Ratchet Wrench	L-TIRW**
Low Torque Indicating Ratchet Wrench Kit	L-TIRWK*

* Contains: RASH3N, RASQ3N, L-TIRW, RTI2035TR, and C9980 adaptor.

** The H-TIRW, L-TIRW, and associated adapters are manufactured by Elos Medtech AB and are distributed by ZimVie Dental.

Drivers, Driver Tips, and Miscellaneous Items

Description	Short	Long
Square Driver	PSQD0N	PSQD1N
Square Driver Tip	RASQ3N	RASQ8N
Small Hexed Driver 0.88 mmD (for cover screw)	PHD00N	PHD01N
Small Hexed Driver Tip 0.88 mmD (for cover screw)	–	RASH7N
Large Hexed Driver 1.2 mmD	PHD02N	PHD03N
Latch-Lock Hex Driver Tip with GemLock Retention 1.2 mm(D)	IHX1.2D	IXL1.2D
Low Profile Abutment Driver	PAD00	PAD24
Low Profile Abutment Driver Tip	RASA3	–
Twist Lock Coping Driver	ICD00	–

Abutment Screws

Description	Gold-Tite	Titanium
Hexed Screw	UNIHG	UNIHT
Square Screw	UNISG	–

For use with PreFormance Posts and Temporary Cylinders, FlexLink TiBase, GingiHue Posts, and UCLA Abutments

Digital Analog Fixation Screw

Description	Item #
Digital Analog Fixation Screw (4 screws in one pack)	ZFX15Z-FS

Laboratory and Impression Coping Screws

Description	Non-Hexed
Try-In Screw (5-pack) 3.4 mmP	MUNITS
Try-In Screw (5-pack) 4.1, 5.0 and 6.0 mmP	UNITS
Waxing Screw/Guide Pin	WSU30

Tapered Implant Surgical Kit

Standard Tapered Ex Hex Bundles

Torque Driver Kits

Description	Item #
Tapered Implant Ex Hex Surgical Kit	TPRDEXHEXKIT
Tapered Implant Ex Hex Surgical Slim Kit	TPRDEXHEXSLMKIT

Components Included in Bundles

Drilling Module

		TPRDEXHEXSLMKIT | Tapered Implant Ex Hex Surgical Slim Kit	TPRDEXHEXKIT | Tapered Implant Ex Hex Surgical Kit
Description	**Item #**		
T3 Pro Surgical Kit, Lid & Base (Empty)	T3PLIDBASE	•	•
Tapered Drilling Module (Empty)	T3PDRILLTRAY	•	•
ACT® Pointed Starter Drill	ACTPSD	•	•
Round Drill	RD100	•	•
Advanced Cutting Technology® (ACT®) Twist Drill 2.0 mm(D) X 10 mm(L)	ACT2010	•	
Advanced Cutting Technology® (ACT®) Twist Drill 2.0 mm(D) X 15 mm(L)	ACT2015	•	•
Advanced Cutting Technology® (ACT®) Twist Drill 2.0 mm(D) X 20 mm(L)	ACT2020	•	
Drill Extender	DEG	•	•
Direction Indicator, 2 mm(D) X 10 mm(L)	DI100	•	•
Quad-Shaping Drill 3.25 mm(D) X 8.5 mm(L)	QSD3285	•	•
Quad-Shaping Drill 3.25 mm(D) X 10 mm(L)	QSD3210	•	•
Quad-Shaping Drill 3.25 mm(D) X 11.5 mm(L)	QSD3211	•	•
Quad-Shaping Drill 3.25 mm(D) X 13 mm(L)	QSD3213	•	•
Quad-Shaping Drill 3.25 mm(D) X 15 mm(L)	QSD3215	•	
Quad-Shaping Drill 4 mm(D) X 8.5 mm(L)	QSD485	•	•
Quad-Shaping Drill 4 mm(D) X 10 mm(L)	QSD410	•	•
Quad-Shaping Drill 4 mm(D) X 11.5 mm(L)	QSD411	•	•
Quad-Shaping Drill 4 mm(D) X 13 mm(L)	QSD413	•	•
Quad-Shaping Drill 4 mm(D) X 15 mm(L)	QSD415	•	
Quad-Shaping Drill 5 mm(D) X 8.5 mm(L)	QSD585	•	
Quad-Shaping Drill 5 mm(D) X 10 mm(L)	QSD510	•	
Quad-Shaping Drill 5 mm(D) X 11.5 mm(L)	QSD511	•	
Quad-Shaping Drill 5 mm(D) X 13 mm(L)	QSD513	•	
Quad-Shaping Drill 5 mm(D) X 15 mm(L)	QSD515	•	
Quad-Shaping Drill 6 mm(D) X 8.5 mm(L)	QSD685	•	
Quad-Shaping Drill 6 mm(D) X 10 mm(L)	QSD610	•	
Quad-Shaping Drill 6 mm(D) X 11.5 mm(L)	QSD611	•	
Quad-Shaping Drill 6 mm(D) X 13 mm(L)	QSD613	•	
Quad-Shaping Drill 6 mm(D) X 15 mm(L)	QSD615	•	
Osseotite NT® Depth Indicator 3.25 mm(D) X 8.5 mm(L)	NTDI3285	•	•
Osseotite NT® Depth Indicator 3.25 mm(D) X 10 mm(L)	NTDI3210	•	•
Osseotite NT® Depth Indicator 3.25 mm(D) X 11.5 mm(L)	NTDI3211	•	•
Osseotite NT® Depth Indicator 3.25 mm(D) X 13 mm(L)	NTDI3213	•	•
Osseotite NT® Depth Indicator 3.25 mm(D) X 15 mm(L)	NTDI3215	•	
Osseotite NT® Depth Indicator 4 mm(D) X 8.5 mm(L)	NTDI485	•	•
Osseotite NT® Depth Indicator 4 mm(D) X 10 mm(L)	NTDI410	•	•
Osseotite NT® Depth Indicator 4 mm(D) X 11.5 mm(L)	NTDI411	•	•

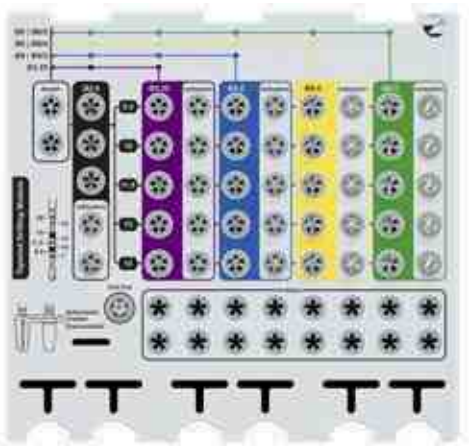

Tapered Implant Slim Surgical Kit

Drilling Module

		TPRDEXHEXSLMKIT	TPRDEXHEXKIT
		Tapered Implant Ex Hex Surgical Slim Kit	Tapered Implant Ex Hex Surgical Kit
Description	**Item #**		
Osseotite NT® Depth Indicator 4 mm(D) X 13 mm(L)	NTDI413	•	•
Osseotite NT® Depth Indicator 4 mm(D) X 15 mm(L)	NTDI415	•	
Osseotite NT® Depth Indicator 5 mm(D) X 8.5 mm(L)	NTDI585	•	
Osseotite NT® Depth Indicator 5 mm(D) X 10 mm(L)	NTDI510	•	
Osseotite NT® Depth Indicator 5 mm(D) X 11.5 mm(L)	NTDI511	•	
Osseotite NT® Depth Indicator 5 mm(D) X 13 mm(L)	NTDI513	•	
Osseotite NT® Depth Indicator 5 mm(D) X 15 mm(L)	NTDI515	•	
Osseotite Nt® Depth Indicator 6 mm(D) X 8.5 mm(L)	NTDI685	•	
Osseotite NT Depth Indicator 6 mm(D) X 10 mm(L)	**NTDI610**	•	
Osseotite NT Depth Indicator 6 mm(D) X 11.5 mm(L)	**NTDI611**	•	
Osseotite NT Depth Indicator 6 mm(D) X 13 mm(L)	**NTDI613**	•	
Osseotite NT Depth Indicator 6 mm(D) X 15 mm(L)	**NTDI615**	•	

ExHex Tooling Module

		TPRDEXHEXSLMKIT	TPRDEXHEXKIT
		Tapered Implant Ex Hex Surgical Slim Kit	Tapered Implant Ex Hex Surgical Kit
Description	**Item #**		
Tapered Implant Ex Hex Tooling Module (Empty)	EXHEXTOOLTRAY	•	•
High Torque Indicating Ratchet Wrench	H-TIRW	•	•
Handpiece Connector	MDR10	•	•
Ratchet Extension 6 mm Long	RE100	•	•
Ratchet Extension 15 mm Long	RE200	•	
Countersink Drill 4.0 mm(D) Implant	ICD100	•	•
Implant Mount 3.4 mm(D) X 15 mm(L)	MMC15	•	•
Narrow Posterior Large Hex Driver-17 mm	PHD02N	•	•
Narrow Posterior Hex Driver-17 mm	PHD00N	•	•
Latch-Lock Hex Driver Tip With Gemlock Retention 1.2 mm(D) 24 mm(L)	IHX1.2D	•	•
Narrow Right Angle Small Hex Driver Tip 24 mm	RASH2N	•	•

Open End Wrench Module

		TPRDEXHEXSLMKIT	TPRDEXHEXKIT
		Tapered Implant Ex Hex Surgical Slim Kit	Tapered Implant Ex Hex Surgical Kit
Description	**Item #**		
Open End Wrench Module (Empty)	OPENWRENCHTRAY	•	•
Open End Wrench	CW100	•	•
Ratchet Wrench	WR150	•	•

Depth Probe Module

	TPRDEXHEXSLMKIT	TPRDEXHEXKIT
	Tapered Implant Ex Hex Surgical Slim Kit	Tapered Implant Ex Hex Surgical Kit
Description	**Item #**	
Depth Probe Module (Empty)	DEPTHGTRAY	•
Implant Depth Gage	DP020	•

T3 PRO Tap Module (T3PTAPMOD)

Description	Item Number
T3 PRO 3.25 mmD and 4 mmD Tap Module (Empty)	T3PTAPTRAY34
T3 PRO 5mmD and 6mmD Tap Module (Empty)	T3PTAPTRAY56
Tapered Implant Dense Bone Tap 3.25 X 8.5mm	NTAP3285
Tapered Implant Dense Bone Tap 3.25 X 10mm	NTAP3210
Tapered Implant Dense Bone Tap 3.25 X 11.5mm	NTAP3211
Tapered Implant Dense Bone Tap 3.25 X 13mm	NTAP3213
Tapered Implant Dense Bone Tap 3.25 X 15mm	NTAP3215
Tapered Implant Dense Bone Tap 4 X 8.5mm	NTAP485
Tapered Implant Dense Bone Tap 4 X 10mm	NTAP410
Tapered Implant Dense Bone Tap 4 X 11.5mm	NTAP411
Tapered Implant Dense Bone Tap 4 X 13mm	NTAP413
Tapered Implant Dense Bone Tap 4 X 15mm	NTAP415
Tapered Implant Dense Bone Tap 5 X 8.5mm	NTAP585
Tapered Implant Dense Bone Tap 5 X 10mm	NTAP510
Tapered Implant Dense Bone Tap 5 X 11.5mm	NTAP511
Tapered Implant Dense Bone Tap 5 X 13mm	NTAP513
Tapered Implant Dense Bone Tap 5 X 15mm	NTAP515
Tapered Implant Dense Bone Tap 6 X 8.5mm	NTAP685
Tapered Implant Dense Bone Tap 6 X 10mm	NTAP610
Tapered Implant Dense Bone Tap 6 X 11.5mm	NTAP611
Tapered Implant Dense Bone Tap 6 X 13mm	NTAP613
Tapered Implant Dense Bone Tap 6 X 15mm	NTAP615
Handpiece Connector	MDR10
Ratchet Extension 6mm Long	RE100
Ratchet Extension 15mm Long	RE200

Parallel Walled Implant Surgical Kits

P = Restorative Platform • D = Diameter • L = Length

PSKT40 (Full Surgical Kit for Parallel Walled Implants)

Parallel Walled Implant Surgical Kits

Description	Item #	PSKT40
Empty Surgical Tray	PTT300I	•
Small Plastic Organizer	PTT100	•
ACT® Reusable Twist Drill, 2.0 mmD x 10 mmL	ACT2010	•
ACT Reusable Twist Drill, 2.0 mmD x 15 mmL	ACT2015	•
ACT Reusable Twist Drill, 2.0 mmD x 20 mmL	ACT2020	•
ACT Reusable Twist Drill, 2.75 mmD x 10 mmL	ACT2710	•
ACT Reusable Twist Drill, 2.75 mmD x 15 mmL	ACT2715	•
ACT Reusable Twist Drill, 2.75 mmD x 20 mmL	ACT2720	•
ACT Reusable Twist Drill, 3.0 mmD x 10 mmL	ACT3010	•
ACT Reusable Twist Drill, 3.0 mmD x 15 mmL	ACT3015	•
ACT Reusable Twist Drill, 3.0 mmD x 20 mmL	ACT3020	•
ACT Reusable Twist Drill, 3.25 mmD x 10 mmL	ACT3210	•
ACT Reusable Twist Drill, 3.25 mmD x 15 mmL	ACT3215	•
ACT Reusable Twist Drill, 3.25 mmD) x 20 mmL	ACT3220	•
ACT Reusable Twist Drill, 3.85 mmD x 10 mmL	ACT3810	•
ACT Reusable Twist Drill, 3.85 mmD x 15 mmL	ACT3815	•
ACT Reusable Twist Drill, 3.85 mmD x 20 mmL	ACT3820	•
ACT Reusable Twist Drill, 4.25 mmD x 8.5 mmL	ACT4285	•
ACT Reusable Twist Drill, 4.25 mmD x 13 mmL	ACT4213	•
ACT Reusable Twist Drill, 4.25 mmD x 18 mmL	ACT4218	•
ACT Reusable Twist Drill, 4.85 mmD x 8.5 mmL	ACT4885	•
ACT Reusable Twist Drill, 4.85 mmD x 13 mmL	ACT4813	•
ACT Reusable Twist Drill, 4.85 mmD x 18 mmL	ACT4818	•
ACT Reusable Twist Drill, 5.25 mmD x 8.5 mmL	ACT5285	•
ACT Reusable Twist Drill, 5.25 mmD x 13 mmL	ACT5213	•
ACT Reusable Twist Drill, 5.25 mmD x 18 mmL	ACT5218	•
ACT Drill Extension	ACTDE	•
Countersink/Pilot Drill, 5.0 mmD	CD500	•
Certain Countersink Drill, 4.0 mmD	ICD100	•
Countersink Depth Indicator for ICD100	ICDI100	•

Description	Item #	PSKT40
Countersink Drill, 4.1 mmD	CD100	•
Countersink/Pilot Drill, 6.0 mmD	CD600	•
Pilot Drill, 2.0-3.0 mmD	PD100	•
Implant Dense Bone Tap, 3.25 mmD x 18 mmL	MTAP2	•
Implant Dense Bone Tap, 4.0 mmD x 13 mmL	TAP413	•
Implant Dense Bone Tap, 5.0 mmD x 13 mmL	TAP53S	•
Implant Dense Bone Tap, 6.0 mmD x 13 mmL	TAP63S	•
Osseotite® 2 Dense Bone Tap, 5.0 mmD x 7-13 mmL	XTAP53S	•
Osseotite 2 Dense Bone Tap, 6.0 mmD x 7-13 mmL	XTAP63S	•
Internal Connection Universal Placement Driver Tip - Long	IIPDTUL	•
Internal Connection Universal Placement Driver Tip - Short	IIPDTUS	•
Certain Universal Ratchet Extension Driver (Short), 6.0 mmL	IRE100U	•
Certain Universal Ratchet Extension Driver (Long), 15 mmL	IRE200U	•
Narrow Posterior Small Hex Driver, 17 mmL	PHD00N	•
Posterior Large Hex Driver - 17 mmL	PHD02N	•
Narrow Right Angle Large Hex Driver Tip - 24 mmL	RASH3N	•
Certain Driver Tip Replacement O-Rings (10-Pack)	IRORDR	•
Handpiece Connector*	MDR10*	•
Open End Wrench (for Ex Hex Implants)	CW100	•
Ratchet Wrench	WR150	•
Ratchet Extension Short 6.0 mmL (For Taps)	RE100*	•
Ratchet Extension Long 15 mmL (For Taps)	RE200*	•
Implant Depth Gauge, 20 mmL	DP020	•
Implant Mount, 3.4 mmP x 15 mmL	MMC15	•
Direction Indicator, 2.0 mmD x 10 mmL 3ea.	DI100	•
Stainless Steel Round Drill, 2.0 mmD	RD100	•

*The Handpiece Connector (MDR10) and the Ratchet Wrench Extensions (RE100, RE200) are used for the Dense Bone Taps and the External Hex Implant Mounts.

High Torque Indicating Ratchet Wrench

Description	Item #
High Torque Indicating Ratchet Wrench	H-TIRW*

* Not included with the PSKT40. The H-TIRW, L-TIRW, and associated adapters are manufactured by Elos Medtech AB and are distributed by ZimVie Dental. Packaged individually.

T3 Short Module (T3SHORTMOD)

Components included in T3SHORTMOD

Description	Item Number
T3 Short Surgical Module (Empty)	T3SHORTTRAY
ACT Pointed Starter Drill	ACTPSD
ACT® Reusable Twist Drill 2.0 mmD x 6.0 mmL	ACT206S
ACT Reusable Twist Drill 3.25 mmD x 6.0 mmL	ACT326S
ACT Reusable Twist Drill 3.85 mmD x 6.0 mmL	ACT386S
ACT Reusable Twist Drill 4.25 mmD x 6.0 mmL	ACT426S
ACT Reusable Twist Drill 4.85 mmD x 6.0 mmL	ACT486S
Flat Bottom Countersink Shaping Drill 3.85 mmD x 5.0 mmL	FCS385S
Flat Bottom Countersink Shaping Drill 3.85 mmD x 6.0 mmL	FCS386S
Flat Bottom Countersink Shaping Drill 4.85 mmD x 5.0 mmL	FCS485S
Flat Bottom Countersink Shaping Drill 4.85 mmD x 6.0 mmL	FCS486S
Short Implant Dense Bone Tap, 5.0 mmD x 5-6.0 mmL	TAP56S
Short Implant Dense Bone Tap, 6.0 mmD x 5-6.0 mmL	TAP66S

NOTE: When placing T3 Short implants, the T3 PRO Surgical Kit must be configured with three specific modules: the ExHex Tooling Module (upper level, housing External Hex-specific drivers and placement tools), the T3 Short Surgical Module, and the Open End Wrench Module (required for final seating). The T3 PRO Kit lid and base are required to house all modules.

Open End Wrench Module

Ex Hex Tooling Module

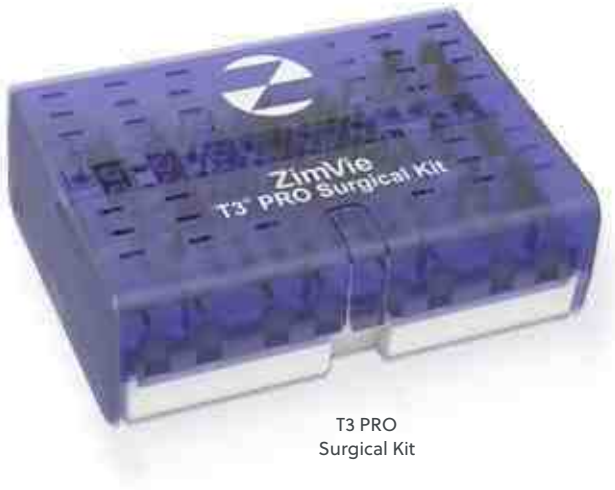

T3 PRO Surgical Kit

For more information, visit ZimVie.com

ZimVie US Corp LLC
4555 Riverside Drive
Palm Beach Gardens, FL 33410
Phone: +1-561-776-6700
Fax: +1-561-776-1272
dentalCS@ZimVie.com

Unless otherwise indicated, as referenced herein, all trademarks and intellectual property rights are the property of ZimVie Inc. and its affiliates; and all products are manufactured by one or more of the dental subsidiaries of ZimVie US Corp LLC (Biomet 3i, LLC, etc.) and distributed by ZimVie US Corp LLC and its authorized marketing partners. H-TIRW and C9980 are manufactured by Elos Medtech Pinol A/S. EU Medical Device classification: dental implants (Class IIb), healing and definitive dental abutments (Class IIb), abutment retaining screws and cover screws (IIb), powered dental instruments (Class IIa), sterile dental instruments (Class Is), dental instruments (Class I). The intended purpose of dental implants is to replace missing individual teeth, multiple teeth, or to restore edentulous dental arches. Healing and definitive abutments are used with endosseous dental implants in the maxilla or mandible to shape soft tissue during healing and to support the final restoration. The intended purpose of cover screws is to seal the implant connection, separating it from soft tissue during healing to prevent tissue ingrowth and allow later placement of restorative components. Abutment retaining screws are intended to mechanically affix a prosthesis to an abutment or an abutment to a dental implant, some retention screws can be used for securing a prosthesis or abutment to an analog during laboratory procedures. Product clearance and availability may be limited to certain countries/regions. This material is intended for clinicians only and does not comprise medical advice or recommendations. Distribution to any other recipient is prohibited.
This material may not be copied or reprinted without the express written consent of ZimVie and is not for distribution in France.
ZVINST0123-GLBL REV C 05/26 ©2026 ZimVie. All rights reserved.

CE 2797